



**Update \_2\_0\_173R**

**Clinical Reminders**

**VA-COVID-19 IMMUNIZATION REMINDER UPDATE  
Install Guide**

**February 2022**

Product Development  
Office of Information Technology  
Department of Veterans Affairs

Table of Contents

<b>INTRODUCTION .....</b>	<b>1</b>
<b>INSTALL DETAILS .....</b>	<b>2</b>
<b>INSTALL EXAMPLE .....</b>	<b>3</b>
<b>POST-INSTALLATION.....</b>	<b>6</b>

# Introduction

---

## DESCRIPTION:

This reminder update will update four template fields used in the VA-SARS-COV-2 IMMUNIZATION reminder dialog and associated progress note template

The Moderna Vaccine has received full FDA approval. The following items were updated, the highlighted items below indicate the changes that were made:

1. Dialog element: VAL-SARS-COV-2 EUA/FDA APPROVAL INFO  
Template field: IM SARS COV-2 INFO TEXT EUA AGES

Vaccine	Age range	Approval
Pfizer-BioNTech COVID-19 Vaccine	16 years and older	FDA Approved
Pfizer-BioNTech COVID-19 Vaccine	5 - 15 years old	EUA
Moderna COVID-19 Vaccine	18 years and older	<b>FDA Approval</b>
Janssen COVID-19 Vaccine	18 years and older	EUA

2. Dialog element: VAL-SARS-COV-2 VACCINE C2 URL  
Template field: IM SARS COV-2 VIS/EUA INFO URL C2  
**Moderna Fact** Sheet for Providers  
Template field: IM SARS COV-2 PROVIDER EUA FACT URL C2  
Moderna **VIS** for Recipients and Caregivers

3. Dialog element: VAL-SARS-COV-2 VACCINE C2 PRE TEXT  
Template field: IM SARS COV-2 ADMIN C2 INFO PRE TEXT

The patient was given the **vaccine information fact sheet** for this vaccine which lists the benefits and side effects of the vaccine and which reviews the risks of the vaccine. The fact sheet was reviewed with the patient and they were given an opportunity to ask questions.

The patient denied any prior severe reaction to this vaccine or its components or a severe allergic reaction such as anaphylaxis to any vaccine or to any injectable therapy.  
The patient gave verbal consent to receive the vaccine.

These three template fields were put in a single new reminder dialog element to make installation easier. It is not necessary to install the dialog component for this update.

Thank you to the following test sites who installed and tested this reminder update:

New Mexico VA Health Care System (Albuquerque)  
VA Nebraska Western Iowa Health Care System  
Ralph J Johnson VA Medical Center (Charleston)  
Aleda E. Lutz VA Medical Center (Saginaw)  
VA Maryland Health Care System (Baltimore)  
VA Bronx

UPDATE\_2\_0\_173R contains 1 Reminder Exchange entry: **UPDATE\_2\_0\_173R VA-COVID-19 IMMUNIZATION REMINDER** with the following components:

#### **TIU TEMPLATE FIELD**

IM SARS COV-2 PROVIDER EUA FACT URL C2  
IM SARS COV-2 ADMIN C2 INFO PRE TEXT  
IM SARS COV-2 VIS/EUA INFO URL C2  
IM SARS COV-2 INFO TEXT EUA AGES

#### **HEALTH FACTORS**

VA-REMINDER UPDATES [C]  
VA-UPDATE\_2\_0\_173R

#### **REMINDER TERM**

VA-REMINDER UPDATE\_2\_0\_173R

#### **REMINDER DIALOG**

VA-SARS-COV-2 173R

## **Install Details**

---


This update is being distributed as a web host file. The address for the host file is:  
**https://REDACTED /UPDATE\_2\_0\_173R.PRD**

The file will be installed using Reminder Exchange, programmer access is not required.  
This update can be loaded with users on the system. Installation will take less than 2 minutes

**YOU SHOULD HAVE INSTALLED THE PRIOR RELEASES (...173O, 173P, 173Q) PRIOR TO INSTALLING THIS UPDATE**

# Install Example

To Load the Web Host File. Navigate to Reminder exchange in Vista

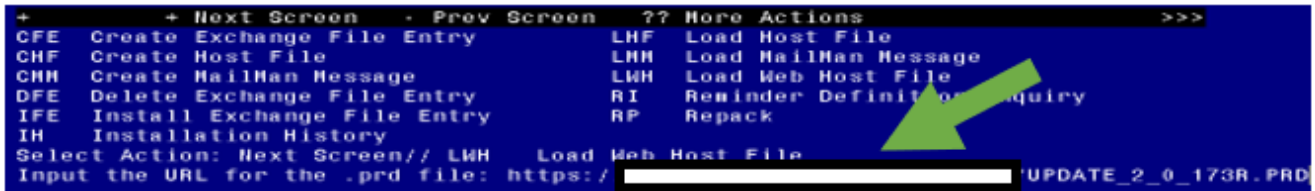

At the **Select Action:** prompt, enter **LWH** for Load Web Host File

At the **Input the url for the .prd file:** prompt, type the following web address:


**https://REDACTED /UPDATE\_2\_0\_173R.PRD** An alternative site that may also have the file is [Index of /Patches\\_By\\_Application/PXRM-CLINICAL REMINDERS/PRD-Files \(worldvista.org\)](https://worldvista.org/Index_of/Patches_By_Application/PXRM-CLINICAL_REMINDERS/PRD-Files)

You should see a message that the file was successfully loaded.



This will install one exchange entry in your exchange file.

Added Reminder Exchange entry UPDATE\_2\_0\_173R VA-COVID-19 IMMUNIZATION REMINDER

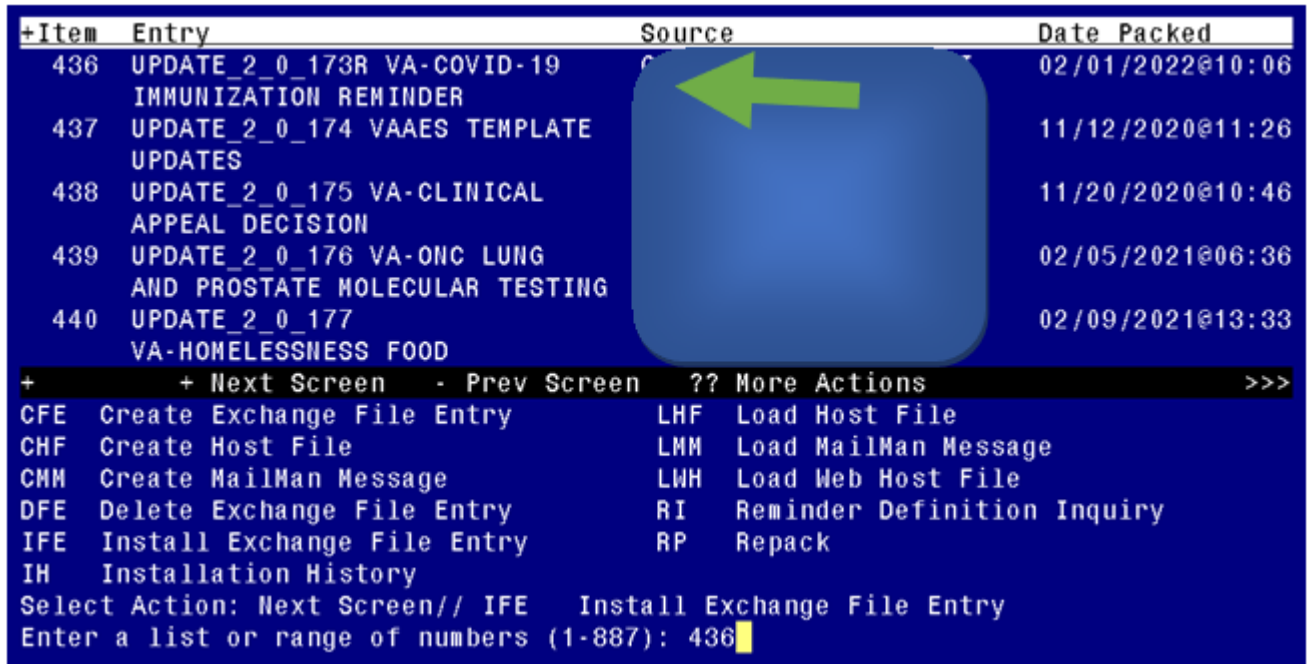

Search and locate an entry titled **UPDATE\_2\_0\_173R VA-COVID-19 IMMUNIZATION REMINDER.**

At the **Select Action** prompt, enter **IFE** for Install Exchange File Entry

Enter the number that corresponds with your entry **UPDATE\_2\_0\_173R VA-COVID-19 IMMUNIZATION REMINDER**. (in this example it is entry 436 it will vary by site). The date of the exchange file should be 02/01/2022.

```
Component Category Exists
Source:
Date Packed: 02/01/2022@10:06:22
Package Version: 2.0P71

Description:
The following Clinical Reminder items were selected for packing:
REMINDER DIALOG
  VA-SARS-COV-2 173R

REMINDER TERM
  VA-REMINDER UPDATE_2_0_173R

Keywords:

Components:

+ Enter ?? for more actions >>>
IA Install all Components IS Install Selected Component
Select Action: Next Screen// IA
```

At the **Select Action** prompt, type **IA** for **Install all Components** and hit enter. Any items that are NEW in any categories, you should **INSTALL**

**Overwrite** the following template fields:  
IM SARS COV-2 PROVIDER EUA FACT URL C2  
IM SARS COV-2 ADMIN C2 INFO PRE TEXT  
IM SARS COV-2 VIS/EUA INFO URL C2  
IM SARS COV-2 INFO TEXT EUA AGES

You will then be prompted to install the reminder dialog component, **you do not need to install this component, choose Q to quit.**

```
Packed reminder dialog: VA-SARS-COV-2 173R
```

Item	Seq.	Dialog Findings	Type	Exist
1		VA-SARS-COV-2 173R Finding: *NONE*	element	

```

+ Next Screen  - Prev Screen  ?? More Actions
DD Dialog Details      DT Dialog Text      IS Install Selected
DF Dialog Findings     DU Dialog Usage    QU Quit
DS Dialog Summary      IA Install All
Select Action: Quit// Q

```

At the **Select Action** prompt, type **Q.**

Component	Category	Exists
Source: [REDACTED]		
Date Packed: 02/01/2022@10:06:22		
Package Version: 2.0P71		
Description:		
The following Clinical Reminder items were selected for packing:		
REMINDER DIALOG		
VA-SARS-COV-2 173R		
REMINDER TERM		
VA-REMINDER UPDATE_2_0_173R		
Keywords:		
Components:		
+      + Next Screen   - Prev Screen   ?? More Actions      >>>		
IA	Install all Components	IS    Install Selected Component
Select Action: Next Screen// 0		

You will then be returned to this screen. At the **Select Action** prompt, type **Q.**

Install complete.

## **Post-Installation**

---

There are no post installation steps required.