



Update_2_0_191

Clinical Reminders

VA-WH OSTEOPOROSIS

Install Guide

March 2021

Product Development
Office of Information Technology
Department of Veterans Affairs

Table of Contents

INTRODUCTION 1
INSTALL DETAILS 2
INSTALL EXAMPLE 3
POST INSTALLATION 6

Introduction

VHA Recommends screening for osteoporosis to prevent osteoporotic fractures with bone measurement testing in:

- Women 65 years and older.
- Postmenopausal women younger than 65 years who are at increased risk for osteoporosis, as determined by a formal clinical risk assessment tool.

The USPSTF concludes that the current evidence is insufficient to assess the balance of benefits and harms of screening for osteoporosis to prevent osteoporotic fractures in men.

Men/Women is determined by the birth sex field in Vista.

Dual energy x-ray absorptiometry (DXA) is the recommended screening method for osteoporosis.

Reminder shows for all women:

- 65 and older without a prior DXA;
- Who haven't had a diagnosis of Osteoporosis within the last two years; and
- Who don't have a code for a terminal condition or documented limited life expectancy

UPDATE_2_0_191 contains 1 Reminder Exchange entry:

UPDATE_2_0_191 VA-WH OSTEOPOROSIS

The exchange file contains the following components:

REMINDER GENERAL FINDINGS

TICKLER REMINDER COMMENT
TICKLER REMINDER

HEALTH FACTORS

VA-REMINDER UPDATES
VA-UPDATE_2_0_191
VA-WH OSTEOPOROSIS
VA-WH OSTEOPOROSIS STOP SCREENING COMORBID
VA-WH OSTEOPOROSIS LIFE EXPECTANCY LESS THAN 5Y
REMINDER FACTORS
LIFE EXPECTANCY < 6 MONTHS
VA-WH OSTEOPOROSIS DECLINE DXA
VA-WH OSTEOPOROSIS ORDER DXA
VA-WH OSTEOPOROSIS DXA SCREEN COMP WRITTEN NO

VA-WH OSTEO DXA SCREEN COMP WRITTEN YES

REMINDER SPONSOR

NATIONAL CENTER FOR HEALTH PROMOTION AND DISEASE
PREVENTION (NCP)
Women Veterans Health Program

REMINDER TAXONOMY

VA-WH OSTEOPOROSIS
VA-TERMINAL CANCER PATIENTS
VA-WH OSTEO DXA COMPLETE

REMINDER TERM

VA-REMINDER UPDATE_2_0_191
VA-WH OSTEO STOP SCREENING
VA-WH OSTEO PATIENT DECLINED
VA-WH OSTEO SCREEN ORDER
VA-WH OSTEO OUTSIDE SCREEN
VA-WH OSTEO SCREEN COMPLETED

REMINDER DEFINITION

VA-WH OSTEOPOROSIS

REMINDER DIALOG

VA-WH OSTEOPOROSIS

Install Details

This update is being distributed as a web host file. The address for the host file is:

https://vaww.va.gov/reminders/docs/UPDATE_2_0_191.PRD

The file will be installed using Reminder Exchange, programmer access is not required.

Installation:

=====

This update can be loaded with users on the system. Installation will take less than 20 minutes.

Install Example

To Load the Web Host File. Navigate to Reminder exchange in Vista

At the **Select Action:** prompt, enter **LWH** for Load Web Host File


At the **Input the url for the .prd file:** prompt, type the following web address:

https://vaww.va.gov/reminders/docs/UPDATE_2_0_191.PRD

You should see a message at the top of your screen that the file successfully loaded.

`https://[redacted]/UPDATE_2_0_191.PRD successfully loaded.`

Search for and locate the reminder exchange entry titled UPDATE_2_0_191 VA-WH OSTEOPOROSIS.

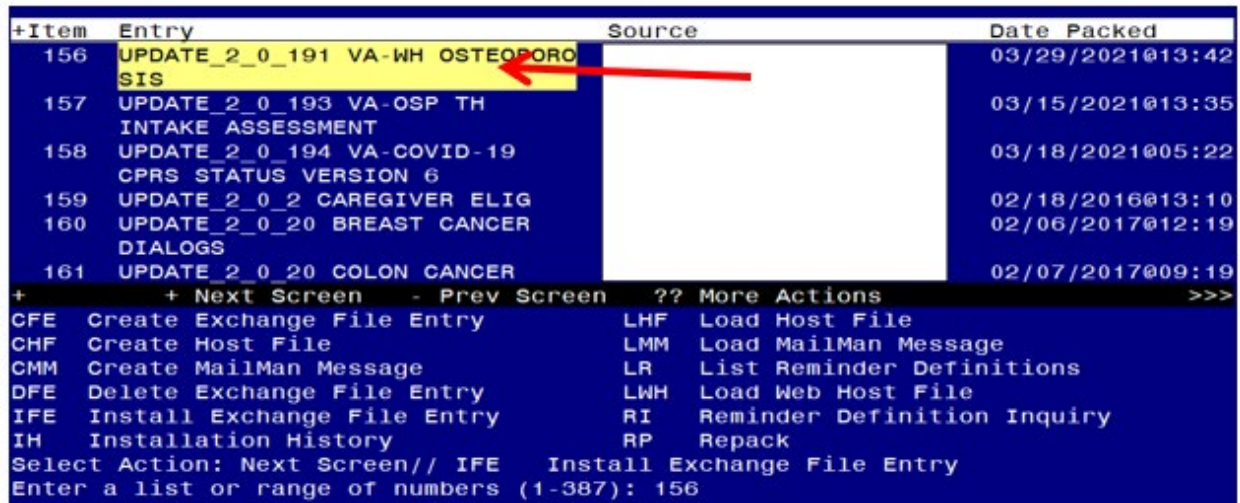

+Item	Entry	Source	Date Packed
156	UPDATE_2_0_191 VA-WH OSTEOPOROSIS		03/29/2021@13:42
157	UPDATE_2_0_193 VA-OSP TH INTAKE ASSESSMENT		03/15/2021@13:35
158	UPDATE_2_0_194 VA-COVID-19 CPRS STATUS VERSION 6		03/18/2021@05:22
159	UPDATE_2_0_2 CAREGIVER ELIG		02/18/2016@13:10
160	UPDATE_2_0_20 BREAST CANCER DIALOGS		02/06/2017@12:19
161	UPDATE_2_0_20 COLON CANCER		02/07/2017@09:19

+	+ Next Screen	- Prev Screen	?? More Actions	>>>
CFE	Create Exchange File Entry	LHF	Load Host File	
CHF	Create Host File	LMM	Load MailMan Message	
CMM	Create MailMan Message	LR	List Reminder Definitions	
DFE	Delete Exchange File Entry	LWH	Load Web Host File	
IFE	Install Exchange File Entry	RI	Reminder Definition Inquiry	
IH	Installation History	RP	Repack	
Select Action: Next Screen// IFE Install Exchange File Entry				
Enter a list or range of numbers (1-387): 156				

At the **Select Action** prompt, enter **IFE** for Install Exchange File Entry

Enter the number that corresponds with your entry titled **UPDATE_2_0_191 VA-WH OSTEOPOROSIS** (in this example it is entry 156, it will vary by site) The date on the exchange file should be 03/29/2021.

```

Component                                     Category      Exists
Source:
Date Packed: 03/29/2021@13:42:13
Package Version: 2.0P46

Description:
The following Clinical Reminder items were selected for packing:
REMINDER DIALOG
  VA-WH OSTEOPOROSIS SCREENING

REMINDER TERM
  VA-REMINDER UPDATE_2_0_191

REMINDER DEFINITION
  VA-WH OSTEOPOROSIS

Keywords:
+ Enter ?? for more actions >>>
IA  Install all Components          IS  Install Selected Component
Select Action: Next Screen// IA

```

At the **Select Action** prompt, type **IA** for Install all Components and hit enter.
 Select Action: Next Screen// **IA Install all Components**

During the installation, you will see several prompts:

Install all new components

SKIP any existing components that you are prompted to overwrite

You will be prompted to install the dialog component:

```

Packed reminder dialog: VA-WH OSTEOPOROSIS SCREENING [NATIONAL DIALOG]

```

Item	Seq.	Dialog Findings	Type	Exists
1		VA-WH OSTEOPOROSIS SCREENING	dialog	
2	5	VA-OSTEO REMINDER INTRO Finding: *NONE*	element	
3	10	VA-GP OSTEO REMINDER OPTIONS Finding: *NONE*	group	
4	10.5	VA-OSTEO SCREENED AFTER 63 Finding: *NONE*	group	
5	10.5.5	VA-OSTEO SCREENED AFTER 63 RECORDS AVAILABLE Finding: VA-WH OSTEO DXA SCREEN COMP WRITTEN YES (HEALTH FACTOR)	element	X
6		PXRM VISIT DATE	prompt	X
7		PXRM DEXA RESULTS	prompt	X
8		PXRM OUTSIDE LOCATION	prompt	X

```

+ Next Screen - Prev Screen ?? More Actions
DD Dialog Details DT Dialog Text IS Install Selected
DF Dialog Findings DU Dialog Usage OU Quit
DS Dialog Summary IA Install All
Select Action: Next Screen// IA

```

At the **Select Action** prompt, type **IA** to install the dialog – **VA-WH OSTEOPOROSIS SCREENING**

Select Action: Next Screen// **IA Install All**

Install reminder dialog and all components with no further changes: **Y// ES**

When you see this prompt, hit enter to link the dialog to the reminder:

Reminder Dialog VA-WH OSTEOPOROSIS SCREENING is not linked to a reminder.

Select Reminder to Link: VA-WH OSTEOPOROSIS//

```

Packed reminder dialog: VA-WH OSTEOPOROSIS SCREENING [NATIONAL DIALOG]
VA-WH OSTEOPOROSIS SCREENING (reminder dialog) installed from exchange file.
Item  Seq. Dialog Findings                               Type  Exists
  1    VA-WH OSTEOPOROSIS SCREENING                      dialog  X
  2    5 VA-OSTEO REMINDER INTRO                          element  X
      Finding: *NONE*
  3    10 VA-GP OSTEOPOROSIS REMINDER OPTIONS             group   X
      Finding: *NONE*
  4    10.5 VA-OSTEO SCREENED AFTER 63                   group   X
      Finding: *NONE*
  5    10.5.5 VA-OSTEO SCREENED AFTER 63 RECORDS AVAILA element  X
      Finding: VA-WH OSTEOPOROSIS SCREEN COMP WRITTEN YES (HEALTH
      FACTOR)
  6    PXRMR VISIT DATE                                  prompt  X
  7    PXRMR DEXA RESULTS                                 prompt  X
  8    PXRMR OUTSIDE LOCATION                            prompt  X
+      + Next Screen  - Prev Screen  ?? More Actions
DD  Dialog Details      DT  Dialog Text      IS  Install Selected
DF  Dialog Findings    DU  Dialog Usage     QU  Quit
DS  Dialog Summary     IA  Install All
Select Action: Next Screen// Q

```

When the dialog has completed installation, you will then be returned to this screen. At the **Select Action** prompt, type **Q**.

```

Component                               Category  Exists
Source:
Date Packed: 03/29/2021@13:42:13
Package Version: 2.0P46

Description:
The following Clinical Reminder items were selected for packing:
REMINDER DIALOG
  VA-WH OSTEOPOROSIS SCREENING

REMINDER TERM
  VA-REMINDER UPDATE_2_0_191

REMINDER DEFINITION
  VA-WH OSTEOPOROSIS

Keywords:
+      + Next Screen  - Prev Screen  ?? More Actions  >>>
IA  Install all Components      IS  Install Selected Component
Select Action: Next Screen// Q

```

You will be returned to this screen. Type Q to quit.
Install Completed

Post Installation

1. Add Order to the reminder dialog
Add your local quick order for dual energy x-ray absorptiometry (DXA) as an additional finding to the element: VA-OSTEO ORDER SCREEN
2. Add this reminder to the cover sheet for the appropriate users. The print name is Osteoporosis Screening.
3. Notify users of this reminder that they need to have the notification Scheduled Alert set to On.
 - a. The tickler alert option in the template will send the user an alert for the date/time that they specify.
 - b. To receive this alert, the scheduled alert notification must be enabled

